

REPLACEMENT SHEET

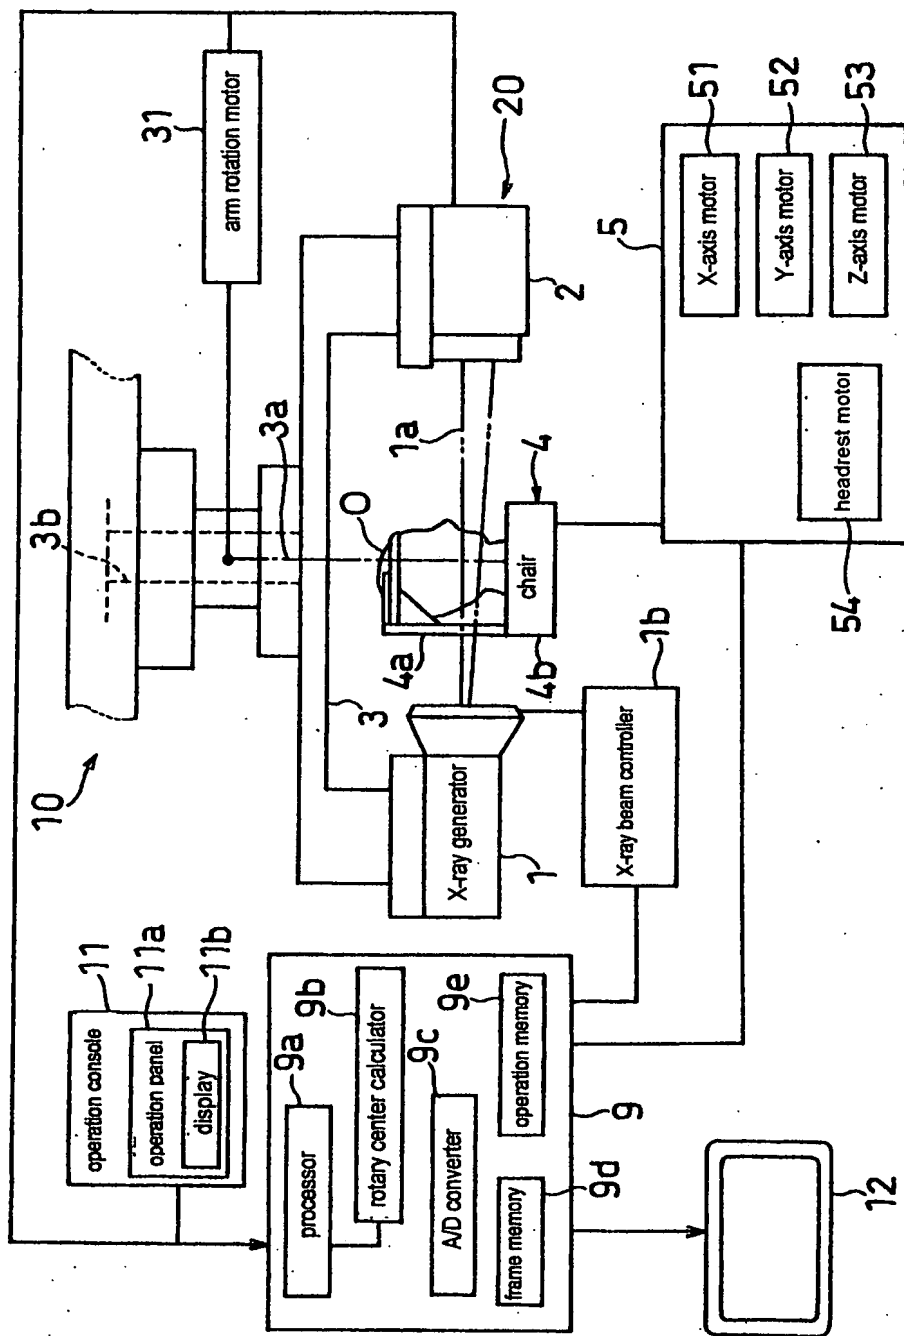


Fig.1

REPLACEMENT SHEET

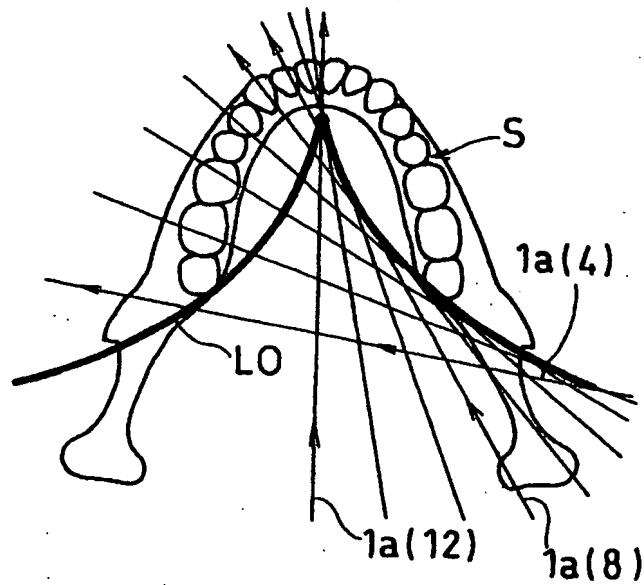


Fig. 2 a

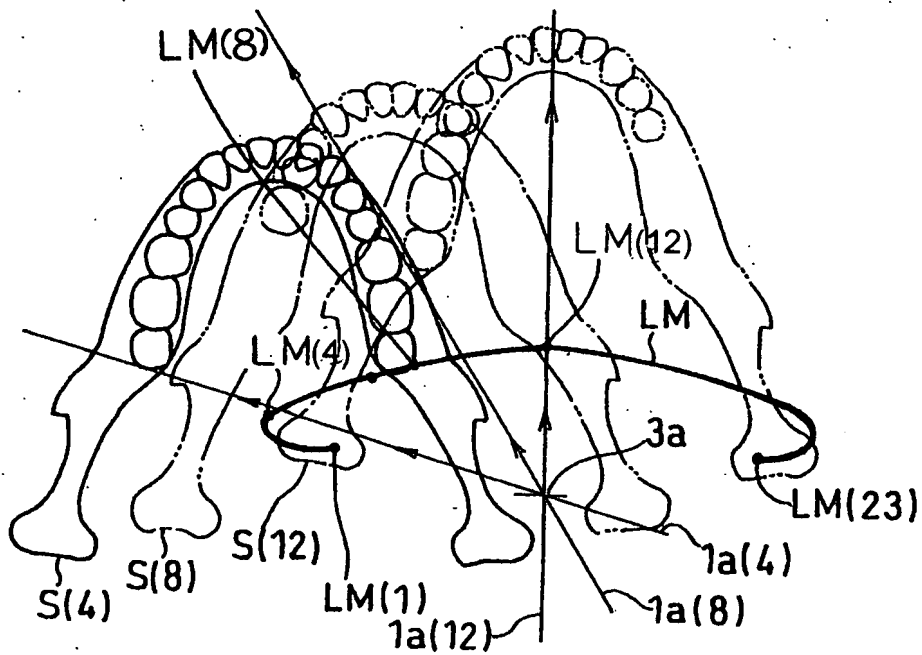


Fig. 2 b

REPLACEMENT SHEET

[CT] 0. 0 sec
 projection method [360 degree projection] 180 degree projection
 copper filter [0. 25mm 0. 5mm 1. 0mm]
 patient size [M]
 imaging area [dental arch]
 80KV
 4.0mA
 slice angle [0 °C]
 Lock

11b
 11c

Fig.4

REPLACEMENT SHEET

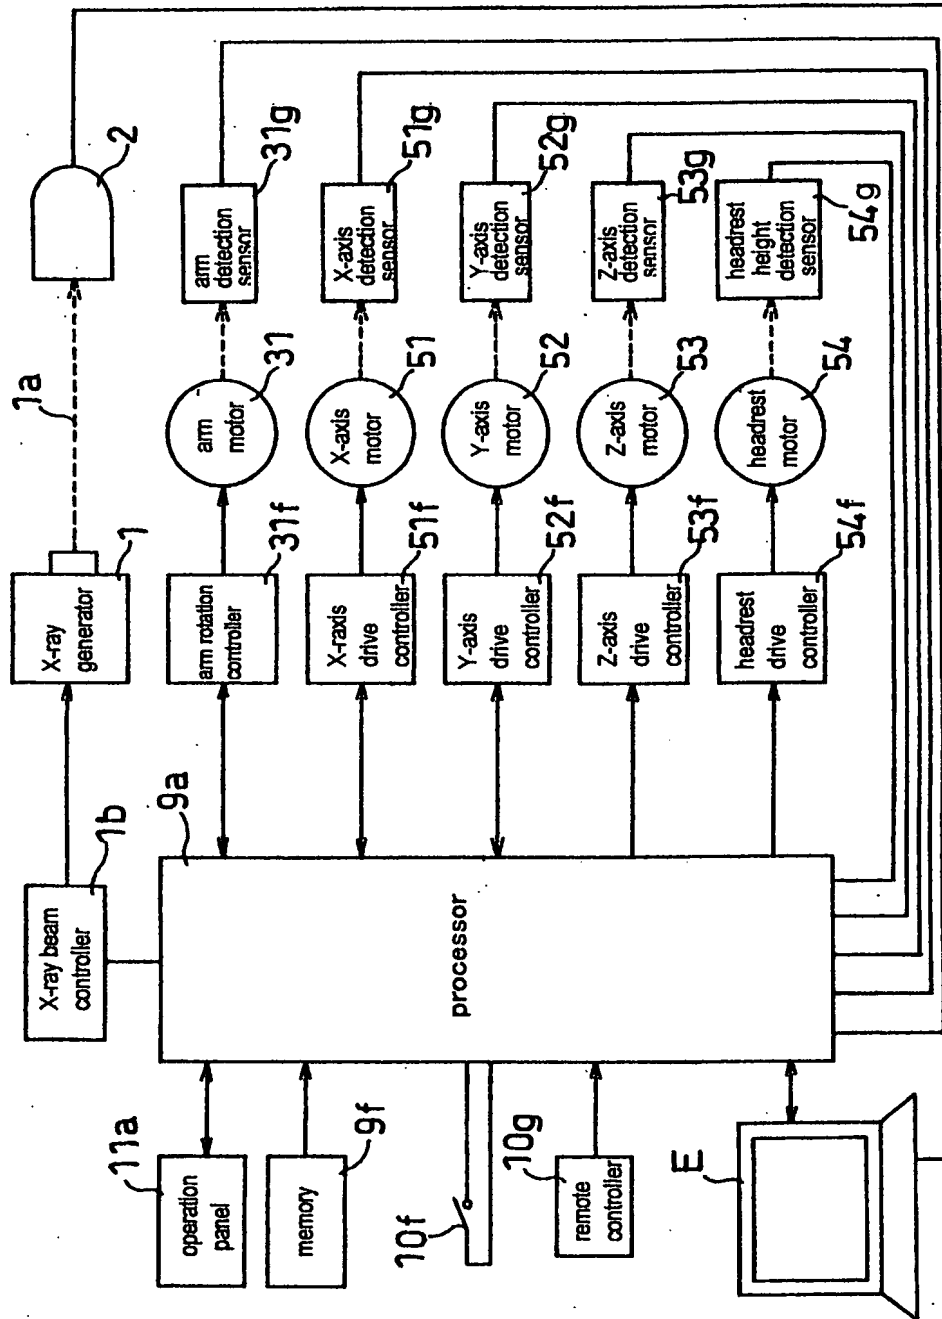


Fig. 9

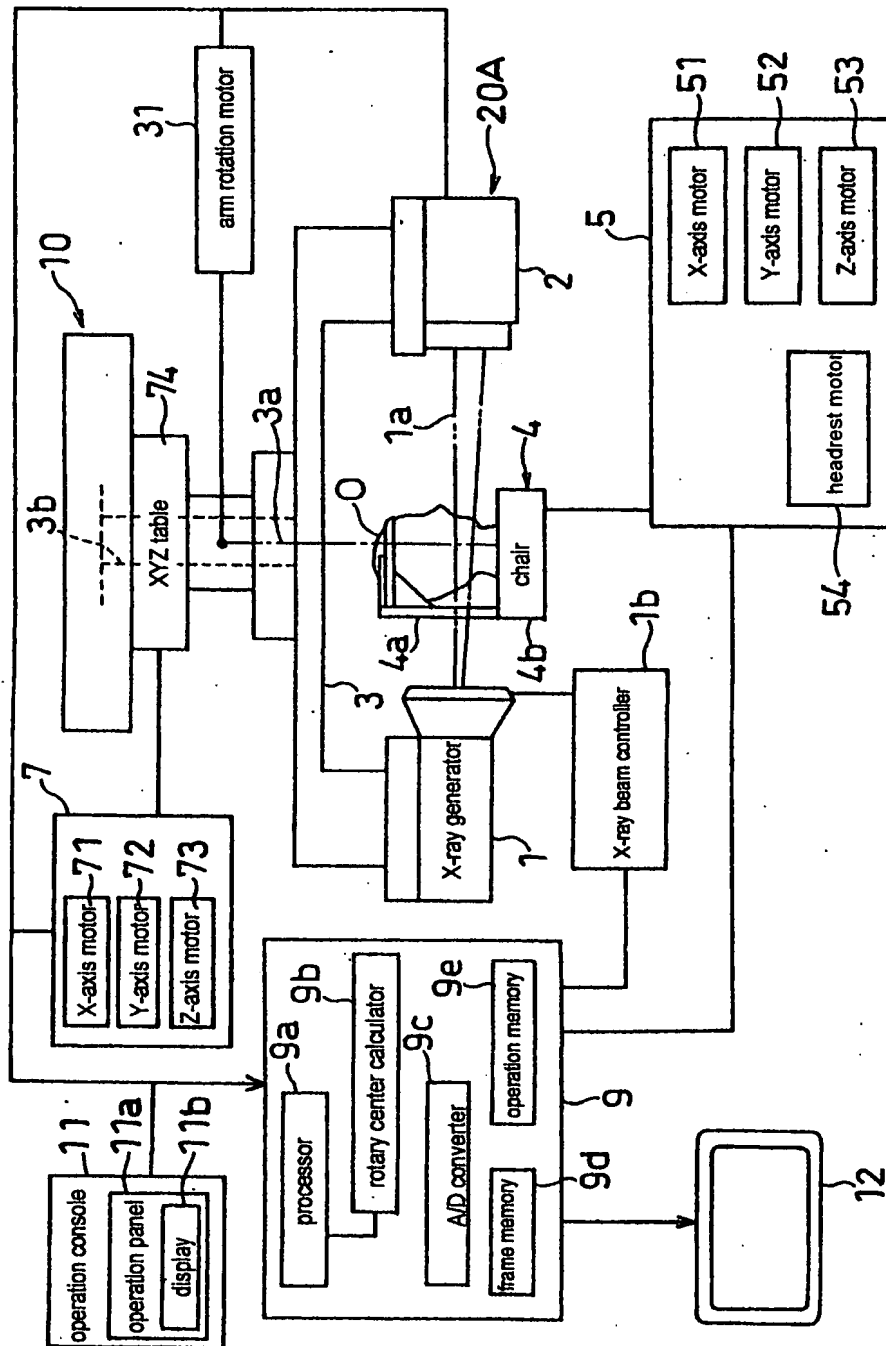


Fig. 14

REPLACEMENT SHEET

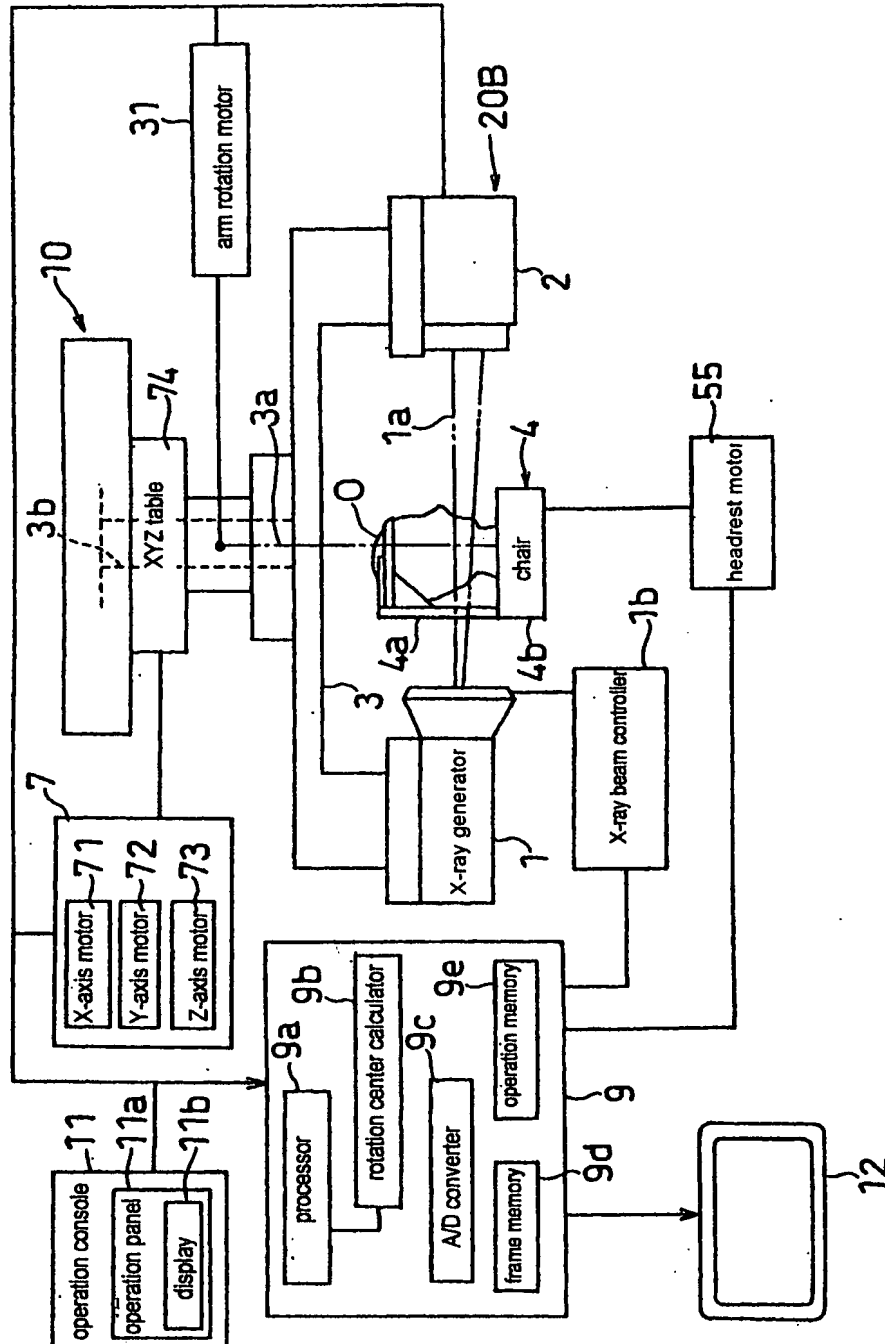


Fig.15